

Summary of Clinical Investigations ES Teck Complex system

EIS System in adjunct to Treatments' monitoring and to diagnosis with the conventional methods

Dr. V. G. Alexeev, Dr. L. V. Kuznekova, Dr E.A. Markelova . Botkin Hospital Moscow
September 25, 2009

Abstract

Clinical investigations were conducted at the S.P. Botkin Hospital from May 20, 2006, to September 1, 2006, in order to evaluate the Bioimpedance parameters provide from a device named Electro Interstitial Scan (E.I.S), we performed drug administration studies.

Two hundred fifteen (215) test subjects (Age 54 ± 16) were recorded with the EIS System.

These patients presented affections diagnosed by conventional examinations (hypothyroidism, hypertension, atherosclerosis or thrombosis risk, and Major depression) and were undergoing no treatment.

The treatments corresponding to the diseases were decided by the conventional examinations results, and a follow-up being undertaken on one hand with the EIS System and on the other hand by conventional methods.

Hypothesis

1. Could the drugs 'administration affect the Bioimpedance parameters estimated from the 3 measured parameters of the EIS system and therefore the EIS can be used in adjunct in treatments' follow up?

2. Could the EIS parameters be used in diagnosis of the diagnosed affections?

The hypothesis 1 was validated according to the raw data analysis:

Thyroid treatment monitoring

The findings show that SDC 11/12 and TSH has a significant negative correlation to each other ($r = -0.975$, $p = 0.005$). It shows that, SDC 11/12 shares approximately 95.1% (that is $(-0.975)^2 \times 100\%$ or $0.951 \times 100\%$) of its variability with TSH. Thus, a high value of SDC 11/12 corresponds to low TSH or low value of SDC 11/12 corresponds to high TSH.

The findings show that EPA-SPA11/12 and TSH has a significant positive correlation to each other ($r = 0.926$, $p = 0.024$). It shows that, EPA-SPA11/12 shares approximately 85.7% (that is $(0.926)^2 \times 100\%$ or $0.857 \times 100\%$) of its variability with TSH. Thus, a high value of EPA-SPA11/12 corresponds to high TSH or low value of EPA-SPA 11/12 corresponds to low TSH.

Beta blockers treatment monitoring

The findings show that SDC 2/4/15/17 and Diastolic Pressure has a significant positive correlation to each other

($r = 0.975$, $p = 0.005$). It shows that, SDC 2/4/15/17 shares approximately 95.1% (that is $(0.975)^2 \times 100\%$ or $0.951 \times 100\%$) of its variability with Diastolic Pressure. Thus, a high value of SDC 2/4/15/17 corresponds to high Diastolic Pressure or low value of SDC 2/4/15/17 corresponds to low Diastolic Pressure.

The findings show that ESGHF/VLF and Diastolic Pressure has a significant positive correlation to each other

($r = 0.977$, $p = 0.004$). It shows that, ESGHF/VLF shares approximately 95.4% (that is $(0.977)^2 \times 100\%$ or $0.954 \times 100\%$) of its variability with Diastolic Pressure. Thus, a high value of ESGHF/VLF corresponds to high Diastolic Pressure or low value of ESGHF/VLF corresponds to low Diastolic Pressure.

ACE inhibitors treatment monitoring

The findings show that EPA-SPA6/8/19/21 and Diastolic Pressure has a significant negative correlation to each other ($r = -0.892$, $p = 0.042$). It shows that, EPA-SPA6/8/19/21/ shares approximately 79.6% (that is $(-0.892)^2 \times 100\%$ or $0.796 \times 100\%$) of its variability with Diastolic Pressure.

Anticoagulant treatment monitoring

The findings show that SDC 6/13/19 and PI (Prothrombin Index) has a significant positive correlation to each other ($r = 0.998$, $p < 0.001$).

The findings show that EPA-SPA 6/13/19 and PI (Prothrombin Index) has a significant positive correlation to each other ($r = 0.961$, $p = 0.009$).

The findings indicate that ESG HF/VLF and PI (Prothrombin Index) has a significant positive correlation to each other ($r = 0.994$, $p = 0.001$).

SSRI treatment monitoring

The findings indicate that there were a significant positive correlations between SDC 9/10 and the treatment Response at D+30 ($\rho = 0.484$, $p < 0.001$) and D+45 and D+60 ($\rho = 0.557$, $p < 0.001$).

The findings indicate that there were a significant positive correlations between EPA-SPA 9/10 and the treatment Response at D+45 ($\rho = 0.709$, $p < 0.001$) and D+60 ($\rho = 0.804$, $p < 0.001$).

2. Could the EIS parameters be used in diagnosis of the affections diagnosed?

The hypothesis 2 was NOT validated according to the raw data analysis:

Only the following correlations had been showed:

The Hypertension group 2A data shows the significant positive correlation between EPA-SPA and Diastolic pressure before the treatment (D).

The major depression group 4 data shows the significant positive correlations between SDC 9/10 and the treatment response (R) for D+ 30 and it also provide evidence of significant positive correlation between ESG HF/VLF and the treatment response (R) for D+45 and D+60 measurements.

**New Approach of Bioimpedance technology concerning
Attention Deficit/Hyperactivity Disorder (ADHD) in Children**

Dr Frederique Caudal (France) , Pr Andrew Stoll USA (Statistical Analysis of the Pre study and power and sample size), Minimax Consulting USA (Statistical analysis of the raw data).

Abstract

Clinical trials were conducted at the office of Dr. Frederique Caudal, paediatrician and specialist in Attention-Deficit/Hyperactivity Disorder (ADHD) in children.

Symptoms of this disorder are related, in the current literature, to a low level of cerebral neurotransmitters.

The diagnosis of ADHD children is almost symptomatic, which leads to the dramatic possibility of error and treatment (Ritalin[®], or SSRI or catecholamine's) with medications associated with numerous side effects in particular for the age of the population.

For this reason, a new, measurable, and therefore objective marker was proposed using the Electro Interstitial Scanner (EIS) Bioimpedance measurement device, in adjunct to the conventional diagnoses and treatment monitoring of the ADHD children.

From 10.04.2006 to 05.16.2007, data from 59 children (age 12 ± 5) presenting ADHD diagnostic and not undergoing treatment were recorded with the EIS System. This database was compared with another control group database (age 14 ± 6) of non-hyperactive children also recorded with the same EIS System.

Hypothesis tested

The hypothesis tested was:

- Can the EIS device with reference to its ESG (Electro Scan Gram) graph be used as a marker for ADHD children and therefore as adjunct to the conventional diagnosis of ADHD children?

This hypothesis was validated by statistical analysis.

Independent Sample T-test

In order to determine the differences between ADHD and the control group in the values of v9/v10, v2/v4/v15/v17 and v1/v3/v16/v18 comparison of means via independent samples t-test was conducted. Table 1.1 presented the t-test results for v9/v10 scores at ADHD and the control group. It shows the number of cases per group used in the analysis, the means, the standard deviation, degrees of freedom, t value and the significance of the test (p-value). The findings in Table 1.1 indicate that the mean of v9/v10 at ADHD (M=78.38) was significantly ($p < 0.001$) higher than the mean of v9/v10 at the control group (M=21.75). Thus, the score of v9/v10 at ADHD was expected to be higher than the scores of v9/v10 at control group.

Table 1.1

Independent Sample T-test for v9/v10 between ADHD and Control

	N	Mean	Std. Deviation	DF	T	P-value
ADHD	104	78.38	30.062	224	19.309	0.000
Control	122	21.75	11.166			

Table 1.2 shows the t-test results for v2/v4/v15/v17 between ADHD and the control group. Accordingly, the mean of v2/v4/v15/v17 at ADHD (M=52.96) was significantly ($p = 0.003$) higher than the mean of v2/v4/v15/v17 at the control group (M=47.96). Thus, the score of v2/v4/v15/v17 at ADHD was expected to be higher than the scores of v2/v4/v15/v17 at the control group.

Table 1.2

Independent Sample T-test for v2/v4/v15/v17 between ADHD and Control

	N	Mean	Std. Deviation	DF	T	P-value
ADHD	208	52.96	19.981	450	3.031	0.003
Control	244	47.96	47.96			

T-test results for v2/v4/v15/v17 between ADHD and the control group were presented in Table 1.3. the findings shows that the mean of v1/v3/v16/v18 at ADHD (M=30.34) was significantly ($p < 0.001$) higher than the mean of v1/v3/v16/v18 at the control group (M=16.75). Thus, the score of v1/v3/v16/v18 at ADHD was expected to be higher than the scores of v1/v3/v16/v18 at the control group.

Table 1.3

Independent Sample T-test for v1/v3/v16/v18 between ADHD and Control

	N	Mean	Std. Deviation	DF	T	P-value
ADHD	208	30.34	1.016	450	12.931	0.000
Control	244	16.57	0.481			

Sensibility and specificity:

Based upon the statistical data analysis, ADHD was correctly predicted at 69% in the group ADHD, and no ADHD was correctly predicted at 89% in the group no ADHD.

Comparing the Accuracy of the Electro Interstitial Scan-Body Composition (EIS-BC) Device between a BC Module and a Valid Assessment of BC and between an EIS Module and a Standard Assessment of Heart Rate Variability

John E. Lewis, Angelica B. Melillo, Evan Long, Yaima Alonso, Elizabeth Ko, Soyona Rafatjah, Janet Konefal, and Judi M. Woolger
Department of Psychiatry and Behavioral Sciences and Department of Medicine University of Miami Miller School of Medicine, Miami, FL 33136

Abstract

The Electro Interstitial Scan-Body Composition (EIS-BC) device consists of two modules: (1) the BC module and (2) the EIS module. The objective of this study was to compare the BC module to a standardized, valid assessment of BC and to compare the EIS module to a standardized assessment of heart rate variability (HRV). Fifty subjects between 20 and 62 years of age were assessed for body composition by the BC module (total body water, fat-free mass, and fat mass) on one hand and dual x-ray absorptiometry (DXA; total fat mass and fat-free mass). On the second hand, spectrum analysis of the EIS module and HRV as measured by a standard HRV device (ES Teck PEMS) to estimate sympathetic nervous system activity were assessed. Height, weight, blood pressure (BP), and pulse were also measured. The results of the study indicated that the correlation between DXA and EIS-BC body fat percent measurements was very high ($r=.92$, $p < 0.001$). The correlation between the EIS spectrum analysis and HRV variables was also very high ($r=.76$, $p < 0.001$), suggesting that the high conductivity ratio has predictive capability on the sympathetic nervous system activity. The results of the study suggest that the EIS-BC device has a significant level of reliability in estimating body composition and sympathetic nervous system activity.

Bioelectrical impedance analysis EIS –BC* versus Quantum II RJL and comparison measurements results and predictive equations used for the 2 devices.**

Dr. V. G. Alexeev, Dr. L. V. Kuznetsova. Botkin Hospital Moscow July, 26 2009

Abstract

Raw Data BC (N=65)

In order to compare the measurements of R, Xc, TWB, FFM and EWC between RJL and EIS-BC paired sample t-test was performed. This test is appropriate when the objective is to compare whether two scores that are taken from the same sample are significantly different. Table 3.3 shows the results of the paired sample t-test for RJL and EIS-BC data, it shows the compared means of each study variables, standard deviation, t-value and the significant value of the test (p-value).

Findings from the paired samples *t* tests in Table 1 were as follows:

- The mean of R at RJL ($M=508.80$) and the mean of R at EIS-BC ($M=509.02$) do not significantly differ. Thus, the scores of R at RJL and R at EIS-BC were statistically equal.
- The mean of Xc at RJL ($M=66.23$) was significantly higher ($p<0.001$) than the mean of Xc at EIS-BC ($M=62.92$). Thus, the scores of Xc at RJL were expected to be higher than the scores of Xc at EIS-BC.
- The mean of TWB at RJL ($M=40.80$) was significantly ($p<0.001$) higher than the mean of TWB at EIS-BC ($M=30.72$). Thus, the scores of TWB at RJL were expected to be higher than the scores of TWB at EIS-BC.
- The mean of FFM at RJL ($M=52.26$) was significantly ($p<0.001$) higher than the mean of FFM at EIS-BC ($M=49.59$). Thus, the scores of FFM at RJL were expected to be higher than the scores of FFM at EIS-BC.
- The mean of EWC at RJL ($M=40.80$) was significantly ($p<0.001$) higher than the mean of EWC at EIS-BC ($M=30.72$). Thus, the scores of EWC at RJL were expected to be higher than the scores of EWC at EIS-BC.

Table 1

Paired Samples T-Test for RJL and EIS-BC data

		Mean	SD	T	P-value
RJL	R	508.8000	71.71868		
EIS-BC	R	509.0154	71.58616	-0.445	0.658
RJL	Xc	66.2308	11.26495		
EIS-BC	Xc	62.9231	10.70238	19.170	0.000
RJL	TWB	40.8046	9.63366		
EIS-BC	TWB	30.7185	7.44830	25.643	0.000
RJL	FFM	52.2569	10.96801		
EIS-BC	FFM	49.5923	10.27891	7.634	0.000
RJL	EWC	16.9769	3.32936		
EIS-BC	EWC	15.5815	2.93991	14.279	0.000

In Conclusion:

Test under raw data BC shows that the scores of Xc, TWB, FFM and EWC for the data RJL were significantly higher than the scores of Xc, TWB, FFM and EWC for the data EIS-BC. Whereas, it also shows that the scores of R for both RJL and EIS-BC data do not show significant difference.

Assessment of Vasoactive Agents and Vascular Aging by the Second Derivative of Photoplethysmogram Waveform

Hypertension: Volume 32(2) August 1998pp 365-370

Takazawa, Kenji; Tanaka, Nobuhiro; Fujita, Masami; Matsuoka, Osamu; Saiki, Tokuyu; Aikawa, Masaru; Tamura, Sinobu; Ibukiyama, Chiharu

Received January 24, 1998; first decision February 8, 1998; revision accepted April 7, 1998.

From The Second Department of Internal Medicine, Tokyo Medical College, Tokyo, Japan.

Abstract

To evaluate the clinical application of the second derivative of the fingertip photoplethysmogram waveform, we performed drug administration studies (study 1) and epidemiological studies (study 2). In study 1, ascending aortic pressure was recorded simultaneously with the fingertip photoplethysmogram and its second derivative in 39 patients with a mean \pm SD age of 54 \pm 11 years. The augmentation index was defined as the ratio of the height of the late systolic peak to that of the early systolic peak in the pulse. The second derivative consists of an a, b, c, and d wave in systole and an e wave in diastole. Ascending aortic pressure increased after injection of 2.5 [μ g] angiotensin from 126/74 to 160/91 mm Hg and decreased after 0.3 mg sublingual nitroglycerin to 111/73 mm Hg. The d/a, the ratio of the height of the d wave to that of the a wave, decreased after angiotensin from -0.40 ± 0.13 to -0.62 ± 0.19 and increased after nitroglycerin to -0.25 ± 0.12 ($P < 0.001$ and $P < 0.001$, respectively). The negative d/a increased with increases in plethysmographic and ascending aortic augmentation indices ($r = 0.79$, $P < 0.001$, and $r = 0.80$, $P < 0.001$, respectively). The negative d/a reflects the late systolic pressure augmentation in the ascending aorta and may be useful for noninvasive evaluation of the effects of vasoactive agents. In study 2, the second derivative of the plethysmogram waveform was measured in a total of 600 subjects (50 men and 50 women in each decade from the 3rd to the 8th) in our health assessment center. The b/a ratio increased with age, and c/a, d/a, and e/a ratios decreased with age. Thus, the second derivative aging index was defined as $b - c - d - e/a$. The second derivative wave aging index (y) increased with age (x) ($r = 0.80$, $P < 0.001$, $y = 0.023x - 1.515$). The second derivative aging index was higher in 126 subjects with any history of diabetes mellitus, hypertension, hypercholesterolemia, and ischemic heart disease than in age-matched subjects without such a history (-0.06 ± 0.36 versus -0.22 ± 0.41 , $P < 0.01$). Women had a higher aging index than men ($P < 0.01$). The b-c-d-e/a ratio may be useful for evaluation of vascular aging and for screening of arteriosclerotic disease. (Hypertension. 1998;32:365-370.)

Summary of the clinical investigations E.S.Teck Complex February, 15, 2011

Bioimpedance /Chronoamperometry in adjunct to screen the prostate cancer with PSA.

Schiavon de Abreu D.
Limeira - SP Brazil

Sponsor
LD Technology LLC

Site of Investigation

Lab Tests:

Labclin Laboratorio de Análises Clínicas
Rua 7 de Setembro, 986
Limeira SP CEP 13480-000 Brazil

Biopsy:

CEAP - CENTRO Especializado em Anatomia Patológica
R. Loefgreen, 625 Vila Clementino - São Paulo
CEP 01040-030 Brazil

Biopsy Analysis

LapMed Anatomia Patológica e Citopatologia
Rua Boa Morte 922 Sala 71
Centro - Limeira SP - Brazil
CEP 13480-182 Brazil

Protocol approved by Brazilian authorities:

Ethics committee: Pesquisa CONEP April, 14 2010 number 125/10

Abstract:

Background: 300 Men were examined for signs and symptoms of prostate disorders. Patients with digital rectal examinations (DRE) indicating positive results were presented for a prostate-specific antigen (PSA) test. A biopsy was advised for 103 of these.

Methods: Only 50 patients reached the last step on the study.

Before undergoing biopsy, an examination with the EPS™ (Electro Prostate Screening) system using bioimpedance and chronoamperometry techniques was performed. Men aged from 49 to 90 years old having an average age of 65 years were included in this study. The EPS™ system uses a direct current (DC) and provides the electrical conductivity and dispersion of 11 pathways of the human body (each of these are recorded twice from anode to cathode, and then, from cathode to anode) between 6 large planar electrodes placed on the palms of the hands, soles of the feet and disposable electrodes are placed on right and left forehead.

Summary of the clinical investigations E.S.Teck Complex February, 15, 2011

In reference to the biopsy results (negative or positive), a statistical analysis of the EPS™ data and PSA was conducted using Roc curves to determine the specificity and sensitivity of each test.

Results: As shown in the results of this investigation for the detection of prostate cancer:

1. The PSA value has a sensitivity of 70.8 % and specificity of 51.9 % with a cut off value > 4 and a sensitivity of 50 % and specificity of 81.5 % with a cutoff value ≥ 5.7 and $p= 0.01$.
2. The delta of the electrical conductivity (DE) of the pathway left foot / right foot has a sensitivity of 62.5 % and specificity of 85.2% with a cutoff value ≤ -5 and $p=0.0001$.
3. The algorithms (ALL= PSA*DE) comprise the delta of electrical conductivity and PSA value have a sensibility of 91.5 % , and a specificity of 59.3 % with a cut off value ≤ -10.52 and $p =0.0003$

Conclusion: Using the PSA reference at least 4.1 ng/ml, the adjunct of the EPS™ system, using bioimpedance and chronoamperometry technologies, to the PSA test could be raised the sensibility from 70.8% to 91.5 % and the specificity from 50% to 85.2 % in prostate cancer screening .

Key words: Prostate cancer screening- Bioimpedance-delta of conductivity - EPS™ system

Comparing the E.S Oxi versus the thoracic impedance (BioZ) for the measurement of the cardiac output

John E. Lewis, Angelica B. Melillo, Evan Long, Yaima Alonso, Elizabeth Ko, Soyona Rafatjah, Janet Konefal, and Judi M. Woolger

Department of Psychiatry and Behavioral Sciences and Department of Medicine University of Miami Miller School of Medicine, Miami, FL 33136

50 patients from 18 to 78 years old were undergoing in simultaneous measurement of the thoracic impedance (gold standard) and E.S Oxi.


150 measurements of cardiac output had been performed with the 2 different devices.

Results:

Correlation

Variable Y	BioZ (Log)
Variable X	ESO (Log)
Sample size	151
Correlation coefficient r	0.8225
Significance level	$P < 0.0001$
95% Confidence interval for r	0.7631 to 0.8682

Summary of the clinical investigations E.S.Teck Complex February, 15, 2011

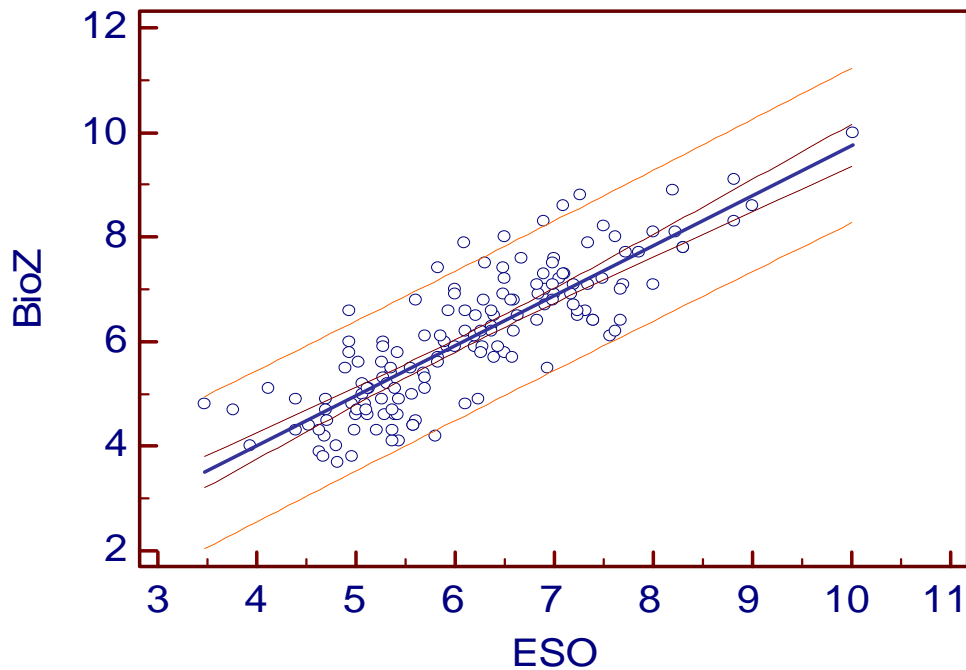

Regression

Dependent Y	BioZ
Independent X	ESO

Sample size	151
Coefficient of determination R ²	0.7027
Residual standard deviation	0.7209

Regression Equation

$y = 0.1742 + 0.9584 x$

Parameter	Coefficient	Std. Error	95% CI	t	P
Intercept	0.1742	0.3202	-0.4585 to 0.8069	0.5440	0.5872
Slope	0.9584	0.05108	0.8575 to 1.0594	18.7652	<0.0001

Analysis of Variance

Source	DF	Sum of Squares	Mean Square
Regression	1	183.0002	183.0002
Residual	149	77.4341	0.5197

F-ratio	352.1320
Significance level	P<0.001

The measurements of the Thoracic impedance BioZ and E.S Oxi have a strong correlation (coefficient of correlation $r=0.82$, coefficient of determination $R^2= 0.70$ and $p < 0.0001$) and therefore the E.S Oxi is validated for the cardiac output measurement.